

Hardline Laboratory

Report No. : HL90578/2020

Page : 1 of 2

Date : NOV. 25, 2020

INTERWORLD NETWORK (M) SDN BHD

G-11 & G-12, KOMPLEKS SEMPILAI, JALAN SEMPILAI, 13700 SEBERANG JAYA, PENANG, MALAYSIA

The following merchandise was submitted and identified by the applicant as:

Product Description: 3 PLY SURGICAL MASK

We have tested the submitted sample(s) as requested and the following results were obtained:

Test Requested: EN 14683:2019 Annex B


Test Method & Result: ---See following sheet(s)---

Date of Receipt: SEP. 26, 2020

Testing Period: SEP. 26, 2020 ~ NOV. 25, 2020

Note: This testing was performed by O.S.H. CO., LTD. Respirator Test Center.

Signed for and on behalf of
SGS Taiwan Ltd.


Sturm Su
Asst. Manager



Test Method & Result:

Test Methods	Test Item	Test Results
1. Testing Sample Number: 5 2. Sample Dimensions : ~9.5 cm x ~17.2 cm 3. Test surface : Outside 4. Test Area: 49 cm ² 5. Flow rate during testing: 28.3 Liter/min 6. Counts of positive control: 1908 CFU 7. Counts of negative control: 0 CFU 8. Average size: 3.2 μm 9. Sample Model: BFE-1090929003	Bacterial filtration efficiency (BFE) (%)	01 >99.9
		02 >99.9
		03 >99.9
		04 >99.9
		05 >99.9

Note :

- The test report merely reflects the test results of the consigned matters of the client and is not a certification.
- The content of this report is invalid if it is not presented as the entire report.

– Picture(s) –

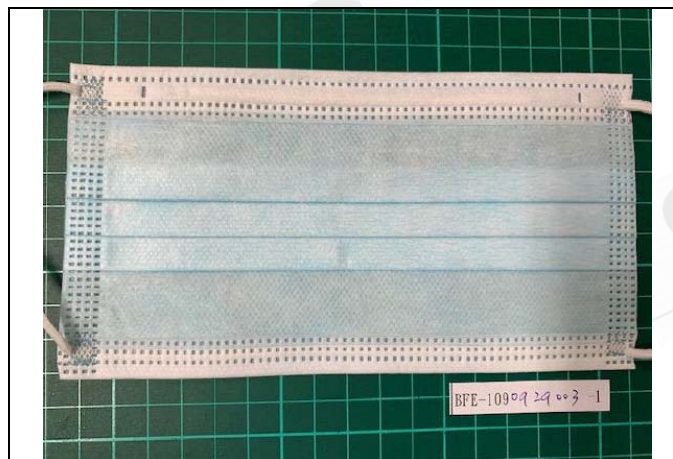


Photo A: Appearance of the sample
- BFE-1090929003

---End of Report---