

Hardline Laboratory

Report No. : HL90581/2020

Page : 1 of 2

Date : OCT. 20, 2020

## INTERWORLD NETWORK (M) SDN BHD

G-11 & G-12, KOMPLEKS SEMPILAI, JALAN SEMPILAI, 13700 SEBERANG JAYA,  
PENANG, MALAYSIA

### The following merchandise was submitted and identified by the applicant as:

Product Description: 3 PLY SURGICAL MASK

### We have tested the submitted sample(s) as requested and the following results were obtained:

Test Requested: ISO 22609:2004


Test Method & Result: ---See following sheet(s)---

Date of Receipt: SEP. 26, 2020

Testing Period: SEP. 26, 2020 ~ OCT. 20, 2020

Note: This testing was performed by O.S.H. CO., LTD. Respirator Test Center.

Signed for and on behalf of  
SGS Taiwan Ltd.

  
Sturm Su  
Asst. Manager



### Test Method & Result:

Test Methods	Test Item		Test Article Number	Synthetic Blood Penetration
1. Testing Sample Number: 32 2. Test Side: Outside 3. Pre-Conditioning : Minimum of 4 hours at (21±5) °C and (85±5) % relative humidity (RH) 4. Test Conditions : 28.4 °C and 35.2 % RH 5. Sample Model: SBP-1090929003	Synthetic Blood Penetration Resistance	120 mmHg (16.0 kPa) As per client requested	01-07、 09-12、14-23、 25-32	None Seen
			8、13、24	Yes

### Note :

1. The test report merely reflects the test results of the consigned matters of the client and is not a certification.
2. The content of this report is invalid if it is not presented as the entire report.

### – Picture(s) –

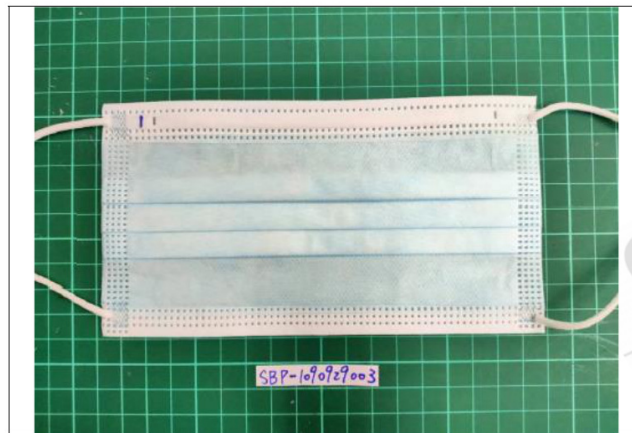


Photo A: Appearance of the sample  
- SBP-1090929003

---End of Report---